

# **Murine Eotaxin ELISA Kit**

Instructions for use

Catalogue numbers: 1x96 tests: 660.060.096

**For research use only**

Fast Track Your Research.....

## Table of Contents

1.	Intended Use .....	2
2.	Introduction.....	2
2.1.	Summary .....	2
2.2.	Principle Of The Method .....	2
3.	Reagents Provided And Reconstitution .....	3
4.	Materials Required But Not Provided .....	3
5.	Storage Instructions.....	4
6.	Specimen Collection, Processing & Storage .....	4
7.	Safety & Precautions For Use .....	5
8.	Assay Preparation .....	6
8.1.	Assay Design.....	6
8.2.	Preparation Of Wash Buffer 1x.....	6
8.3.	Preparation Of Assay Buffer 1x .....	6
8.4.	Preparation Of Standard.....	7
8.5.	Preparation Of Biotin-Conjugate.....	7
8.6.	Preparation Of Streptavidin-HRP.....	7
9.	Method .....	8
10.	Data Analysis.....	9
11.	Assay Limitations.....	9
12.	Performance Characteristics .....	10
12.1.	Sensitivity .....	10
12.2.	Specificity .....	10
12.3.	Precision.....	10
12.4.	Dilution Parallelism .....	10
12.5.	Spike Recovery .....	10
12.6.	Stability.....	10
12.7.	Expected Serum Values .....	10
13.	Assay Summary .....	11

# Murine Eotaxin ELISA KIT

## 1. Intended use

The murine Eotaxin ELISA kit is a solid phase sandwich ELISA for the *in-vitro* qualitative and quantitative determination of mEotaxin in supernatants, buffered solutions or serum samples. This assay will recognise both natural and recombinant mEotaxin.

**This kit has been configured for research use only. Not suitable for use in therapeutic procedures.**

## 2. Introduction

### 2.1. Summary

Eotaxin, also known as CCL11, is a member of the CC chemokine family of inflammatory and immunoregulatory cytokines.

Constitutive Eotaxin mRNA expression has been detected in multiple tissues, most often it appears to be induced by inflammatory cytokines such as IL-1, TNF $\alpha$  and IFN $\gamma$  in fibroblasts, endothelial and epithelial cells. Following allergen challenge Eotaxin mRNA has been shown to be rapidly up-regulated in airway epithelium and alveolar macrophages. Eotaxin expression has also been detected in smooth muscle cells, chondrocytes and eosinophils.

Mouse Eotaxin activity is mediated by the mouse CC chemokine receptor CCR3, which, unlike human CCR3, can also be activated by mouse MIP-1 $\alpha$ .

Among CC chemokine family members, Eotaxin is functionally and structurally mostly related to the MCP/Eotaxin proteins. Mouse Eotaxin cDNA encodes a 97 amino acid residue precursor protein that is cleaved to generate the 74 aa residue mature protein.

Mouse Eotaxin has been shown to be a potent chemoattractant for eosinophils during inflammation and allergic reactions and to be involved in the growth of myeloid cell progenitors and the differentiation of mast cells during embryonic development. A role in numerous eosinophil-associated gastrointestinal disorders as food allergy, parasitic infections, allergic colitis and inflammatory Bowel disease has been described.

### 2.2. Principle of the method

A capture Antibody highly specific for mEotaxin has been coated to the wells of the microtiter strip plate provided during manufacture. Binding of mEotaxin samples and known standards to the capture antibodies and subsequent binding of the biotinylated anti-mEotaxin secondary antibody to the analyte is completed during the same incubation period. Any excess unbound analyte and secondary antibody is removed.

The HRP conjugate solution is then added to every well including the zero wells, following incubation excess conjugate is removed by careful washing.

A chromogen substrate is added to the wells resulting in the progressive development of a blue coloured complex with the conjugate. The colour development is then stopped by the addition of acid turning the resultant final product yellow. The intensity of the produced coloured complex is directly proportional to the concentration of mEotaxin present in the samples and standards.

The absorbance of the colour complex is then measured and the generated OD values for each standard are plotted against expected concentration forming a standard curve. This standard curve can then be used to accurately determine the concentration of mEotaxin in any sample tested.

### 3. Reagents provided and reconstitution

Reagents (Store@2-8°C)	Quantity 1x96 well kit Cat no. 660.060.096	Reconstitution
96-well microtiter strip plate	1	Ready to use (Pre-coated)
Plastic plate covers	2	n/a
mEotaxin Standard: 4 ng/ml	2	Reconstitute as directed on the vial (see Assay preparation, section 8)
Sample Diluent	1 (12ml)	Ready to use
Assay buffer	1 (5 ml)	20x Concentrate, dilute in distilled water (see Assay preparation, section 8)
Biotin Conjugate anti-mEotaxin	1 (70µl)	Dilute in Assay Buffer 1X (see Assay preparation, section 8)
Streptavidin-HRP	1 (150µl)	Dilute in Assay Buffer 1X (see Assay preparation, section 8)
Wash Buffer	1 (50ml)	20x Concentrate, dilute in distilled water (see Assay preparation, section 8)
Substrate Solution	1 (15ml)	Ready to use
Stop Solution	1 (15ml)	Ready to use

### 4. Materials required but not provided

- Microtiter plate reader fitted with appropriate filters (450 nm required with optional 620 nm reference filter)
- Microplate washer or wash bottle
- 10, 50, 100, 200 and 1,000µl adjustable single channel micropipettes with disposable tips
- 50-300µl multi-channel micropipette with disposable tips
- Multichannel micropipette reagent reservoirs
- Distilled water
- Vortex mixer
- Miscellaneous laboratory plastic and/or glass, if possible sterile

## 5. Storage Instructions

Store kit reagents between 2 and 8°C. Immediately after use remaining reagents should be returned to cold storage (2-8°C). Expiry of the kit and reagents is stated on box front labels. The expiry of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, the reagent is not contaminated by the first handling.

**Wash Buffer 1X:** Once prepared, store at 2-8°C for up to 30 days.

**Assay Buffer 1X:** Once prepared, store at 2-8°C for up to 30 days.

**Reconstituted Standard:** Once prepared use immediately and do not store.

**Diluted Biotin conjugate :** Once prepared use immediately and do not store.

**Diluted Streptavidin-HRP:** Once prepared use immediately and do not store.

## 6. Specimen collection, processing & storage

Cell culture supernatants and serum were tested with this assay. Other biological samples might be suitable for use in the assay. Remove serum from the clot or red cells, respectively, as soon as possible after clotting and separation.

**Cell culture supernatants:** Remove particulates and aggregates by spinning at approximately 1000 x g for 10 min.

**Serum:** Use pyrogen/endotoxin free collecting tubes. Serum should be removed rapidly and carefully from the red cells after clotting. Following clotting, centrifuge at approximately 1000 x g for 10 min and remove serum.

**Storage:** If not analysed shortly after collection, samples should be aliquoted (250-500µl) to avoid repeated freeze-thaw cycles and stored frozen at -70°C. Avoid multiple freeze-thaw cycles of frozen specimens.

**Recommendation:** Do not thaw by heating at 37°C or 56°C. Thaw at room temperature and make sure that sample is completely thawed and homogeneous before use. When possible avoid use of badly haemolysed or lipemic sera. If large amounts of particles are present these should be removed prior to use by centrifugation or filtration.

## 7. Safety & precautions for use

- Handling of reagents, serum or plasma specimens should be in accordance with local safety procedures, e.g. CDC/NIH Health manual : "Biosafety in Microbiological and Biomedical Laboratories" 1984.
- Laboratory gloves should be worn at all times.
- Avoid any skin contact with Stop solution and Substrate Solution. In case of contact, wash thoroughly with water.
- Do not eat, drink, smoke or apply cosmetics where kit reagents are used.
- Do not pipette by mouth.
- When not in use, kit components should be stored refrigerated as indicated on vials or bottles labels.
- All reagents should be warmed to room temperature before use. Lyophilized standards should be discarded after use.
- Once the desired number of strips has been removed, immediately reseal the bag to protect the remaining strips from deterioration.
- Cover or cap all reagents when not in use.
- Do not mix or interchange reagents between different lots.
- Do not use reagents beyond the expiration date of the kit.
- Use a clean disposable plastic pipette tip for each reagent, standard, or specimen addition in order to avoid cross contamination, for the dispensing of Stop Solution and Substrate Solution, avoid pipettes with metal parts.
- Use a clean plastic container to prepare the washing solution.
- Thoroughly mix the reagents and samples before use by agitation or swirling.
- All residual washing liquid must be drained from the wells by efficient aspiration or by decantation followed by tapping the plate forcefully on absorbent paper. Never insert absorbent paper directly into the wells.
- The Substrate Solution is light sensitive. Avoid prolonged exposure to light. Also, avoid contact of the Substrate Solution with metal to prevent colour development. Warning Substrate Solution is toxic avoid direct contact with hands. Dispose off properly.
- If a dark blue colour develops within a few minutes after preparation, this indicates that the Substrate solution has been contaminated and must be discarded. Read absorbance's within 1 hour after completion of the assay.
- When pipetting reagents, maintain a consistent order of addition from well-to-well. This will ensure equal incubation times for all wells.
- Follow incubation times described in the assay procedure.
- Dispense the Substrate Solution within 15 min of the washing of the microtiter plate.

## 8. Assay Preparation

Bring all reagents to room temperature before use

### 8.1. Assay Design

Determine the number of microwell strips required to test the desired number of samples plus appropriate number of wells needed for running zeros and standards. Each sample, standard and zero should be tested **in duplicate**. Remove sufficient microwell strips for testing from the pouch immediately prior to use. Return any wells not required for this assay with desiccant to the pouch. Seal tightly and return to 2-8°C storage.

**Example plate layout** (example shown for a 6 point standard curve)

	Standards		Sample Wells									
	1	2	3	4	5	6	7	8	9	10	11	12
A	2000	2000										
B	1000	1000										
C	500	500										
D	250	250										
E	125	125										
F	62.5	62.5										
G	zero	zero										
H												

*All remaining empty wells can be used to test samples in duplicate*

### 8.2. Preparation of Wash Buffer 1X

Pour entire contents (50 ml) of the Wash Buffer Concentrate (20x) into a clean 1000 ml graduated cylinder. Bring to final volume of 1000 ml with glass-distilled or deionized water. Mix gently to avoid foaming.

Transfer to a clean wash bottle and store at 2° to 25°C.

### 8.3. Preparation of Assay Buffer 1X

Pour the entire contents (5 ml) of the Assay Buffer Concentrate (20x) into a clean 100 ml graduated cylinder. Bring to final volume of 100 ml with distilled water. Mix gently to avoid foaming.

Store at 2° to 8°C.

## 8.4. Preparation of Standard

Standard vials must be reconstituted with the volume of distilled water shown on the vial immediately prior to use. This reconstitution gives a stock solution of 4 ng/ml of mEotaxin. Mix the reconstituted standard gently by inversion only. Serial dilutions of the standard are made directly in the assay plate to provide the concentration range from 2000 to 62.5 pg/ml. A fresh standard curve should be produced for each new assay.

- Add 100µl of Sample Diluent to all standard wells and zeros.
- Immediately after reconstitution add 100µl of the reconstituted standard to wells A1 and A2, which provides the highest concentration standard at 2000pg/ml.
- Transfer 100µl from wells A1 and A2 to B1 and B2. Mix the well contents by repeated aspirations and ejections taking care not to scratch the inner surface of the wells.
- Continue this 1:1 dilution using 100µl from wells B1 and B2 through to wells F1 and F2 providing a serial diluted standard curve ranging from 2000pg/ml to 62.5pg/ml.
- Discard 100µl from the final wells of the standard curve (F1 and F2).

Alternatively these dilutions can be performed in separate clean tubes and immediately transferred into the relevant wells.

## 8.5. Preparation of Biotin-Conjugate

**Please note that the Biotin-Conjugate should be used within 30 minutes after dilution.**

Make a 1:100 dilution of the concentrated **Biotin-Conjugate** solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

Number of Strips	Biotin-Conjugate (ml)	Assay Buffer (1x) (ml)
1 - 6	0.03	2.97
1 - 12	0.06	5.94

## 8.6. Preparation of Streptavidin-HRP

**Please note that the Streptavidin-HRP should be used within 30 minutes after dilution.**

Make a 1:100 dilution of the concentrated **Streptavidin-HRP** solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

Number of Strips	Streptavidin-HRP (ml)	Assay Buffer (1x) (ml)
1 - 6	0.06	5.94
1 - 12	0.12	11.88



## 9. Method

We strongly recommend that every vial is mixed thoroughly without foaming prior to use.

Prepare all reagents as shown in section 8.

**Note:** Final preparation of Biotin conjugate (section 8.5) and Streptavidin-HRP (section 8.6) should occur immediately before use.

Assay Step		Details
1.	Wash	a) Dispense 0.4 ml of <b>1x washing solution</b> into each well b) Aspirate the contents of each well c) Repeat steps a and b
2.	Addition	<b>Prepare Standard curve</b> as shown in section 8.4
4.	Addition	Add 50µl of <b>Sample diluent</b> and 50µl of <b>Sample</b> in duplicate to appropriate number of wells
5.	Addition	Add 50µl of diluted <b>biotin-conjugate</b> to all wells
6.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for <b>2 hour(s)</b> if available on a microplate shaker set at 400 rpm
7.	Wash	Remove the cover and wash the plate as follows: a) Aspirate the liquid from each well b) Dispense 0.4 ml of <b>1x washing solution</b> into each well c) Aspirate the contents of each well d) Repeat step b and c another three times
8.	Addition	Add 100µl of diluted <b>Streptavidin-HRP</b> into all wells
9.	Incubation	Cover with a plastic plate cover and incubate at room temperature (18 to 25°C) for <b>1 hour</b> if available on a microplate shaker set at 400 rpm
10.	Wash	Repeat wash step 7.
11.	Addition	Add 100µl of ready-to-use <b>Substrate Solution</b> into all wells
12.	Incubation	Incubate in the dark for <b>10 minutes*</b> at room temperature. Avoid direct exposure to light by wrapping the plate in aluminium foil.
13.	Addition	Add 100µl of <b>Stop Solution</b> into all wells
<p><b>Read the absorbance</b> value of each well (immediately after step 13.) on a spectrophotometer using 450 nm as the primary wavelength and optionally 620 nm as the reference wave length (610 nm to 650 nm is acceptable).</p>		

*\*Incubation time of the substrate solution is usually determined by the ELISA reader performance. Many ELISA readers only record absorbance up to 2.0 O.D. Therefore the colour development within individual microwells must be observed by the analyst, and the substrate reaction stopped before positive wells are no longer within recordable range.*

## 10. Data Analysis


Calculate the average absorbance values for each set of duplicate standards, controls and samples. Ideally duplicates should be within 20% of the mean.

Create a standard curve by plotting the mean absorbance for each standard concentration on the ordinate against the mouse Eotaxin concentration on the abscissa. Draw a best fit curve through the points of the graph (a 5-parameter curve fit is recommended).

The amount of mEotaxin in each sample is determined by extrapolating OD values against mEotaxin standard concentrations using the standard curve.

### Example mEotaxin Standard curve

Standard	mEotaxin concentration (pg/ml)	OD (450nm) mean	CV (%)
1	2000	2.228	5.0
2	1000	1.543	3.1
3	500	0.991	1.4
4	250	0.554	5.0
5	125	0.326	1.3
6	62.5	0.177	1.0
zero	0	0.039	9.2

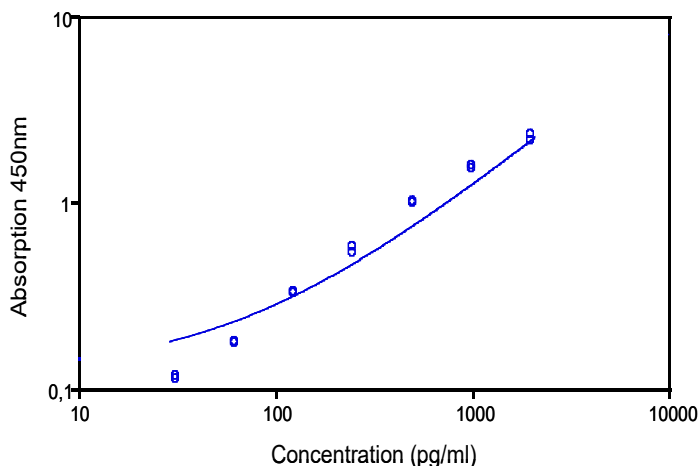

**Note:** curve shown above should not be used to determine results. Every laboratory must produce a standard curve for each set of microwell strips assayed.

For samples human serum or plasmas which have been diluted 1:2 according to the protocol, the calculated concentration should be multiplied by the dilution factor (x2).

## 11. Assay limitations

Do not extrapolate the standard curve beyond the maximum standard curve point. The dose-response is non-linear in this region and good accuracy is difficult to obtain. Concentrated samples above the maximum standard concentration must be diluted with Standard diluent or with your own sample buffer to produce an OD value within the range of the standard curve. Following analysis of such samples always multiply results by the appropriate dilution factor to produce actual final concentration.

The influence of various drugs on end results has not been investigated. Bacterial or fungal contamination and laboratory cross-contamination may also cause irregular results.

Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing fresh Washing Buffer, fill with Washing Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.

Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.

As with most biological assays conditions may vary from assay to assay therefore **a fresh standard curve must be prepared and run for every assay.**

## 12. Performance Characteristics

### 12.1. Sensitivity

The limit of detection of murine Eotaxin defined as the analyte concentration resulting in an absorbance significantly higher than that of the dilution medium (mean plus 2 standard deviations) was determined to be 3.6 pg/ml (mean of 6 independent assays).

### 12.2. Specificity

The interference of circulating factors of the immune system was evaluated by spiking these proteins at physiologically relevant concentrations into a murine Eotaxin positive serum.

There was no crossreactivity detected.

### 12.3. Precision

#### Intra-assay

Reproducibility within the assay was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 8 serum samples containing different concentrations of murine Eotaxin. 2 standard curves were run on each plate. **The calculated overall intra-assay coefficient of variation was 5.6%.**

#### Inter-assay

Assay to assay reproducibility within one laboratory was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 8 serum samples containing different concentrations of murine Eotaxin. 2 standard curves were run on each plate. **The calculated overall inter-assay coefficient of variation was 9.4%.**

### 12.4. Dilution Parallelism

Serum samples with different levels of murine Eotaxin were analysed at serial 2 fold dilutions with 4 replicates each.

**The recovery ranged from 103% to 121% with an overall recovery of 114%.**

### 12.5. Spike Recovery

The spike recovery was evaluated by spiking 4 levels of murine Eotaxin into serum. Recoveries were determined in 3 independent experiments with 6 replicates each. The unspiked serum was used as blank in these experiments.

**The overall mean recovery was 66%.**

### 12.6. Stability

#### Storage Stability

Aliquots of serum samples were stored at -20°C, 2-8°C, room temperature (RT) and at 37°C, and the murine Eotaxin level determined after 24 h. There was no significant loss of murine Eotaxin immunoreactivity detected during storage under above conditions.


#### Freeze-thaw Stability

Aliquots of serum samples were stored at -20°C and thawed 5 times, and the murine Eotaxin levels determined. There was no significant loss of murine Eotaxin immunoreactivity detected by freezing and thawing.

### 12.7. Expected serum values

A panel of 6 serum pools from randomly selected apparently healthy mice was tested for murine Eotaxin. The detected murine Eotaxin levels ranged between 98 and 236 pg/ml with a mean level of 176 pg/ml. The levels measured may vary with the sample collection used.

## 13. Assay Summary

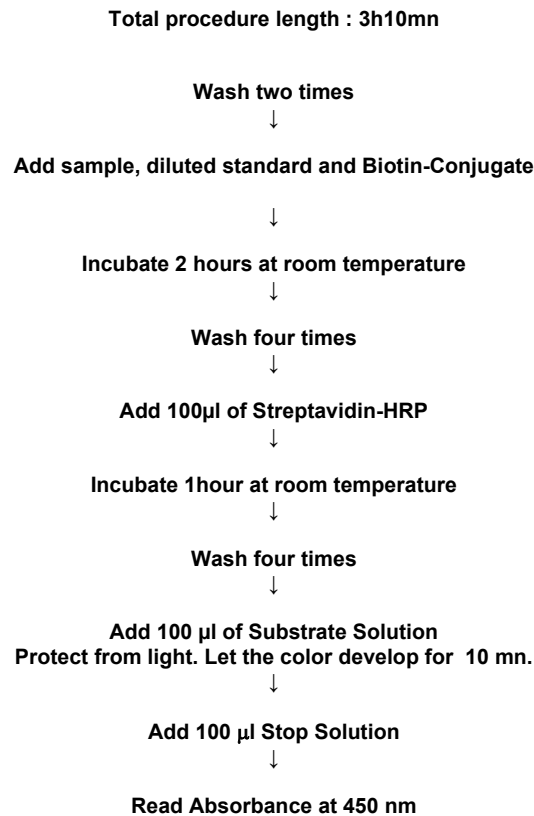

### Supplier:

Diaclone SAS  
6 Rue Dr Jean-François-Xavier Girod  
25000 Besançon  
France  
Tel +33 (0)3 81 41 38 38  
Email: [techsupport@medixbiochemica.com](mailto:techsupport@medixbiochemica.com)